


# Indicator Calibration

## i-Checker IC2000 SERIES 170

- The i-Checker makes it easier to continuously perform high-accuracy inspection of various indicators.
- A wide variety of optional accessories enable the inspection and calibration of many types of gages including dial indicators, lever-type dial indicators, dial test indicators, bore gages, Digimatic indicators, linear gages and lever gage heads that use various stem diameters and support systems.
- Can directly inspect indicators with a stroke of up to 100 mm.
- The pointer of the analog indicator is positioned just before the measuring point automatically in the semi-automatic mode.
- Digital indicators equipped with a data output function are checked very efficiently due to spindle positioning at the inspection points and recording of measurement results being under fully automatic control.

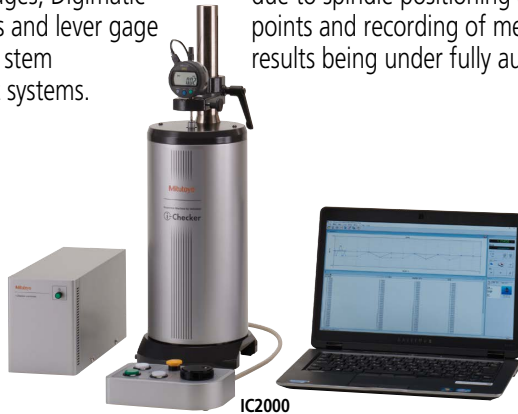


IC2000

### SPECIFICATIONS


Code No.	170-402	170-403
Measuring Range	100 mm	
Resolution	0.01 μm	
Accuracy (20 °C)	vertical orientation (0.1 + 0.4L/100) μm L=Arbitrary length (mm) lateral orientation (0.15 + 0.6L/100) μm L=Arbitrary length (mm)	
Feed speed	Maximum 10 mm/s	
Drive method	Motor drive (semi-automatic/fully-automatic)	
Measuring Unit	Separate type Linear Encoder	
Measurement method	Semi-automatic measurement	
	Fully automatic measurement (only when using an indicator equipped with data output function)*1*2	
Mass	20 kg	
Operating temperature	20 °C±0.5 °C	
Remarks	with 8 mm bush	with 3/8 in bush

\*1 Automatic measurement requires the indicator's connection cable. Additionally some form of indicator, along with the normally connected accessory (the optional accessory for the indicator such as a Digimatic power-supply unit in an EF counter) will be required.

\*2 The indicator measured via RS-232C has the capability to receive data from the main unit and output the counter value.

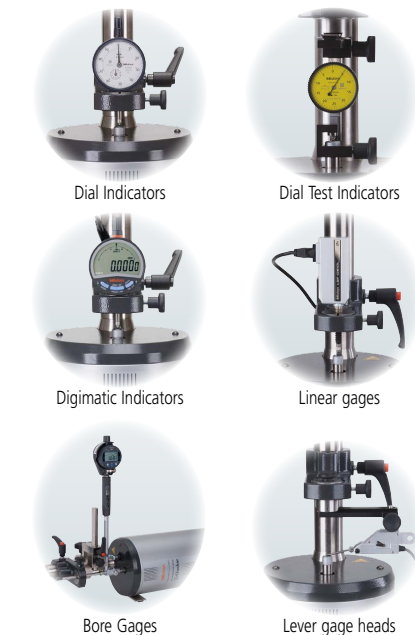

### DIMENSIONS

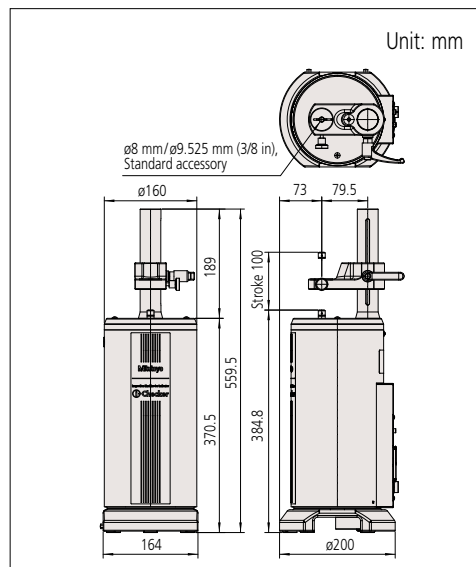

### Typical application for Dial Test Indicator Accessory Set



Typical application using dial test indicator attachment set (02ASK000)

